

cT 10SG Reagent Strips Urinalysis dip and read strips for visual test

Tests for : Blood, Bilirubin, Urobilinogen, Ketones(acetoacetic acid), Protein, Nitrite, Glucose, pH, Specific Gravity and Leukocytes in urine.

⚠ WARNINGS AND PRECAUTIONS:

cT 10SG Reagent Strips are for *in vitro* diagnostic use and are intended for professional use. The "universal precautions" recommended by the Centers for Disease Control should be adhered to whenever blood or body fluids are handled.¹ These precautions include wearing gloves.

cT 10SG urine test strips may contain either diazonium salt or nitroferrocyanide. Avoid contact with skin and mucous membranes; flush affected areas with copious amounts of water. Get immediate medical attention for eyes or if ingested. Exercise the normal precautions required for handling all laboratory reagents.

SUMMARY AND INTENDED USE:

cT 10SG reagent strip is a dip - and - read test strip and intended for use as an *in vitro* diagnostic aid using urine specimens. The strip contains solid phase reagent areas affixed to a plastic support and is provided in a dry reagent format. This strip provides tests for, qualitatively and semiquantitatively, occult blood, bilirubin, urobilinogen, ketones(acetoacetic acid), protein, nitrite, glucose, pH, specific gravity and leukocytes by the visual comparison with color charts of each concentration range. No additional reagents or laboratory equipment is required. The reagent strips are packaged in a plastic vial containing desiccant. The test strips must be tightly capped in the plastic vial to assure reagent reactivity. The directions must be followed exactly, and it is necessary to use **fresh, well-mixed and uncentrifuged** urine for optimal results.

CHEMICAL PRINCIPLES OF THE PROCEDURE:

Blood: This test is based on the pseudoperoxidase activity of hemoglobin which catalyzes the reaction of O-Tolidine and buffered organic peroxide, Cumene hydroperoxide. The resulting color ranges from yellow green through green to dark green.

Bilirubin: This test is based on the coupling of bilirubin with 2,4-dichlorobenzene diazonium Na in a strong acid medium. The color changes from light tan to purple.

Urobilinogen: The test is based on the diazotization reaction of 4-methoxybenzene diazonium salt and urinary urobilinogen in a strong acid medium. The color changes range from pink to brown-red.

Ketones: This test is based on the reaction of acetoacetic acid in the urine with nitroprusside. The resulting color ranges from tan when no reaction takes place to purple for positive reaction.

protein: This test is based on the color change of the indicator, tetrabromophenol blue, in the presence of protein. A positive reaction is indicated by a color change from yellow through green and then to greenish - blue.

Nitrite: This test is based on the reaction of p - arsanilic acid and nitrite (which is derived from dietary nitrate in the presence of bacteria) in urine to form a diazonium compound. The diazonium compound in turn couples with N-(1- naphthyl)ethylenediamine 2HCl in an acidic medium. The resulting color is pink. Any degree of pink color is considered positive.

Glucose: This test is based on a sequential enzyme reaction. First, glucose oxidase catalyzes the formation of gluconic acid and hydrogen peroxide from the oxidation of glucose. A second enzyme, peroxidase, catalyzes the reaction of hydrogen peroxide with potassium iodide chromogen to oxidize the chromogen to colors ranging from blue through greenish - brown and brown to dark - brown.

pH: This test is based on double indicators (methyl red and bromothymol blue) which give a broad range of colors covering the entire urinary pH range. Colors range from orange through greenish - yellow and green to blue.

Specific Gravity: This test is based on the pKa change of certain pretreated polyelectrolytes in relation to ionic concentration. In the presence of an indicator, color range from deep blue in urine of low ionic concentration through green and yellow - green in urines of increasing ionic concentration.

Leukocytes: This test reveals the presence of granulocyte esterases. The esterases cleave an derivatized thiazole amino acid ester to liberate derivatized hydroxy thiazole. This thiazole then reacts with a diazonium salt to produce a purple product.

REAGENTS: (Based on dry weight at the time of impregnation of 100 strips)

Blood	Cumene hydroperoxide	7.00 mg
	O - Tolidine	3.00 mg
Bilirubin	2,4 - Dichlorobenzenediazonium Na	3.0 mg
	Oxalic acid	30.0 mg
Urobilinogen	4 - Methoxybenzenediazonium salt	2.5 mg
	Citric acid	30.0 mg
Ketones	Sodium nitroprusside	20.0 mg
	Magnesium sulfate	246.5 mg
Protein	Tetrabromophenol blue	0.3 mg
	Citric acid	110.0 mg
	Sodium citrate	46.0 mg
Nitrite	p - Arsanilic acid	5.0 mg
	N-(1-naphthyl)ethylenediamine 2HCl	6.0 mg
Glucose	Glucose oxidase	451 unit
	Peroxidase	186 unit
	Potassium iodide	10.0 mg
pH	Methyl red	0.04 mg
	Bromothymol blue	0.5 mg
Specific Gravity	Bromothymol blue	1.2 mg
	Diethylenetriaminepentaacetic acid	12.0 mg
Leukocytes	Phenylthiazole amino acid ester	1.0 mg
	Diazonium salt	0.7 mg

CDP-CT10(R0)

STORAGE:

Store at room temperature between 2°C - 30°C (38°F - 86°F). Do not store the strips in the refrigerator or freezer. Cap the bottle tightly. Since the test strips are sensitive to specific environmental factors, such as moisture, heat and light, do not expose strips to these factors.

PROCEDURE FOR HANDLING THE STRIPS:

All unused strips must be stored in the original bottle. Do not remove desiccant from bottle. Transfer of the strips to another container may cause reagent strips to deteriorate and become unreactive. After taking out test strips, replace the cap promptly and tightly. Do not touch test area of the strip. Do not use strips after expiration date. The work area should be clean and free of detergents and other contaminants.


SPECIMEN COLLECTION AND PREPARATION:

Use a clean, dry, unused vessel to collect the urine. Test the urine as soon as possible after collection. If testing cannot be done within an hour after voiding, refrigerate the specimen immediately and let it return to room temperature before testing.

PROCEDURE:

This procedure **MUST BE FOLLOWED EXACTLY** to achieve reliable test results.

1. Confirm that the product is within the expiration date shown on the label.
2. Remove the strip from the bottle and replace the cap immediately.
3. Inspect the strip. Discoloration or darkening of reagent areas may indicate deterioration. Do not use the strip.

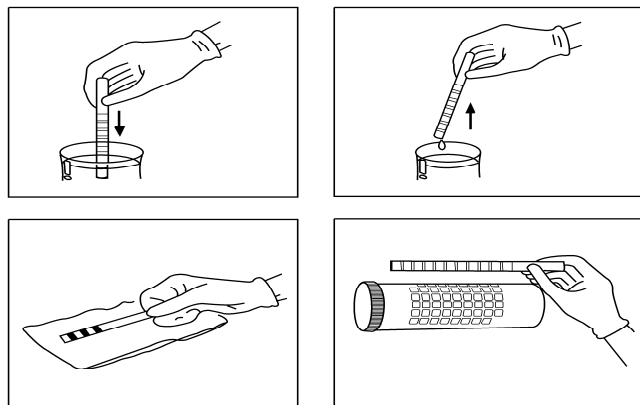

4. Dip the test strip completely for no more than 1 second in fresh, well-mixed, and uncentrifuged urine specimen. Excessive urine on the test strip may give rise to a wrong result. Remove the excessive urine by touching the plastic film on the rim of vessel. At this time, do not allow the reagent areas to touch the rim of vessel. Excessive urine may be removed by gently blotting the lengthwise edge on absorbent paper.
5. Compare the test results carefully with the color chart on the bottle label in good light. Proper reading time (30 - 60 seconds) is critical for optimal results. While comparing, keep the strip in a horizontal position to avoid possible interaction of chemicals by excessive urine. Changes in color that appear only along the edges of the test areas or after more than two minutes have passed are of no diagnostic significance.

QUALITY CONTROL:

The strips must be properly stored and handled before and during the testing. Reaction of reagent strips should be confirmed by testing known positive and negative specimens or multiple analyte controls containing normal and abnormal amounts of each of the analytes being tested.

RESULTS:

The results are obtained by direct comparison of test strip with the color blocks printed on the bottle label. No calculations or laboratory instruments are necessary.

LIMITATIONS OF PROCEDURES:

Substances that cause abnormal urine color, such as drugs containing azo dyes, nitrofurantoin and riboflavin may affect the readability of reagent areas on urinalysis reagent strips.

The color development on the reagent pad may be masked, or a color reaction may be produced on the pad that could be interpreted visually and instrumentally as a false positive. It is therefore recommended that in case of doubt, the test should be repeated after withdrawal of the medication.

Blood: A false positive can sometimes occur when bacteria are present in the urine. Ascorbic acid or protein may reduce the reactivity of the blood test. Strong oxidizing substances, such as hypochlorites, may produce a false positive result. Urine from menstruating females often, but not always, yields positive results.

Bilirubin: Normally no bilirubin is detectable in urine by even the most sensitive methods. Since the bilirubin in specimens is sensitive to light, exposure of the urine specimens to light for a long period time may result in a false negative. Ascorbic acid concentration of 25 - 50mg/dl may also cause false negatives. Even trace amounts of bilirubin are sufficiently abnormal to require further investigation. False positive results may be obtained in the presence of diagnostic or therapeutic dyes in the test urine.

Urobilinogen: A complete absence of urobilinogen in the specimen being tested cannot be demonstrated by the strip. Normal urine specimens ordinarily give a slight pink color. Higher concentration of formalin may give false negative result. This test is not a reliable method for the detection of urobilinogen.

Ketones: Normal urine specimens ordinarily yield negative results with this reagent. False positive results may occur with highly pigmented urine specimens or those containing large amounts of levodopa metabolites.²

Protein: The minimum sensitivity of this test is 5 - 10mg/dl of protein in urine. Highly buffered alkaline urines (pH 9) may give false positive results.² The interpretation of results is also difficult in turbid urine specimens.

Nitrite: Any degree of uniform pink color development should be considered positive, however, pink spots or pink edges should not be interpreted as a positive result. Color development is not proportional to the number of bacteria present. The nitrite test detects only nitrate reducing bacteria. Occasionally bacteria will be present that do not reduce nitrate to nitrite. Therefore, a negative, therefore, a mid stream of first morning urine specimen is recommended for this test.² Sensitivity of the nitrite test is decreased with high specific gravity or ascorbic acid concentrations of 25mg/dl or greater.

Glucose: Reactivity of the test decreases as the specific gravity and/or pH of urine increases, and may also vary with temperature. Ascorbic acid (more than 50mg/dl) and ketone bodies (more than 40mg/dl) may cause a false negative for a specimen containing a small amount of glucose (100mg/dl), however, the combinations of such ketone levels and low glucose levels are metabolically improbable in screening.

pH: This pH test indicates the pH values only within the range of 5 to 9. Certain drugs, such as those used for hypertension and heart trouble (Acetazolamides) may cause alkaline urine.² Excessive urine on the test strip may wash the acid buffer from the neighboring protein reagent onto the pH area and change the pH reading to an acid pH although the urine being tested is originally neutral or alkaline. This is called the 'run-over' phenomenon.

Specific Gravity: Elevated specific gravity readings may be obtained in the presence of moderate quantities (100mg - 700mg/dl) of protein, specific gravity is increased with the glucose in the urine.

Leukocytes: The test result may not always be consistent with the leukocyte cell number by the microscopic examination.⁵ Positive results may be found high humidity and high temperature condition, and failure of the bottle security. Positive results may occasionally be found with the random specimens from females due to contamination of the specimens by the vaginal discharge. High concentration of glucose, high specific gravity, high level of albumin, high concentration of formaldehyde, or presence of blood may cause decreased test results. High concentration of oxalic acid or trace of oxidizing agents may cause false negative results. Low specific gravity (1,010 and under) may cause a false positive.

EXPECTED VALUES:

Blood: Hemolysis is a natural process of recycling old or damaged red cells. But when hemoglobin appears in urine, it indicates some kind of kidney disease or some kind of urinary tract disorder. The practical detection limit of this test is approximately 5 to 10 erythrocytes per microliter of urine. Blood is often, but not always, found in the urine of menstruating females. This test is highly sensitive to hemoglobin (it is slightly less so to intact erythrocytes) and thus complements the microscopic examination.

Bilirubin: No bilirubin is detectable in urine of healthy persons by even the most sensitive methods. Elevated bilirubin in urine always indicates disease and is the earliest sign of liver cell disease and/or biliary obstruction. The signs of "+" (0.5mg/dl), "++" (1.0mg/dl), and "+++" (3.0mg/dl) signify the qualitative severity of the liver damage or bile obstruction. Even trace amounts of bilirubin are sufficiently significant to require further investigation.

Urobilinogen: In this test strip, the normal urobilinogen range is 0.1 to 1.0mg/dl (1mg/dl is approximately equal to 1 Ehrlich unit/dl).³ If results exceed the concentration of 2.0mg/dl, the patient and/or the urine specimen should be evaluated further.

Ketones: Ketone bodies should not be detected in normal urine specimens with this reagent. The concentrations given: "±" (5mg/dl), "+" (15mg/dl), "++" (40mg/dl), "+++" (80mg/dl) correlate well with the acetoacetic acid concentration in urine. The sensitivity of this test is 5mg acetoacetic acid per 100ml of urine. Detectable levels of ketone may occur with frequent vomiting, diarrhea, digestive disturbances, pregnancy, or severe physical exercise.⁴

Protein: Normal urine specimens ordinarily contain some protein (0 - 4mg/dl); therefore, only persistent elevated levels of urine protein indicate kidney or urinary tract disease. The persistent results of trace level or over indicates significant proteinuria, and thus further clinical testing is needed to evaluate the significance of results. The concentrations given: "+" (30mg/dl); "++" (100mg/dl); "+++" (300mg/dl); "++++" (1000mg/dl) correlate well with the albumin concentrations in urine. Pathologic proteinuria generally gives values above 30mg/dl and is persistent.

Nitrite: Testing of urine for nitrite tests for bacteria in urine. Any degree of pink color after 30 seconds indicates clinically significant bacteriuria. Bacteriuria is generally due to infection of the kidneys, ureters, bladder or urethra.

Glucose: Normally no glucose is detectable in urine, although a minute quantity of glucose is excreted by the normal kidney. Approximately 50-100mg glucose/dl of urine is detectable in this test strip. Concentrations of 100mg/dl may be considered as abnormal if found consistently.

pH: Normal urine is slightly acid with a pH of 6, and urine pH values generally range from 5 to 8 pH units. The pH of urine is an important indicator of certain metabolic, kidney, gastrointestinal and respiratory factors.

SPECIFIC GRAVITY: Random urine specimens from adults may vary in specific gravity from 1.003 to 1.040. Twenty-four hour urines from normal adults with normal diets and normal fluid intake will have a specific gravity of 1.016 - 1.022. This test permits determination of urine SG between 1.000 and 1.030.

Leukocytes: Normally no leukocytes are detectable in urine. Individually observed trace results may be questionable clinical significant.

PERFORMANCE CHARACTERISTICS:

Specific performance characteristics of the cT 10SG products are based both on clinical and laboratory studies. A study done at two clinical sites involving 94 patient samples compared cT 10SG to a competitor's strip. 100% agreement within one color block was obtained for all analytes except protein. Protein gave a greater than 95% agreement. The lower agreement may be reflective of the technician's interpretation of the negative versus trace color block with both the cT 10SG and the competitive strip. Parameters of importance to the user are sensitivity, limits of test, specificity, accuracy, precision and stability. Sensitivity and limits of tests are the generally detectable levels of each test described previously. The sensitivity depends upon several factors; the variability of color perception; the presence or absence of inhibitory factors typically found in urine, the specific gravity, ascorbic acid, and pH; and lighting conditions when the product is read visually. The tests have been developed to be specific for the constituent to be measured with the exception of interferences listed previously. Exact agreement between visual results and instrumental results might not be found because of the inherent differences between the perception of the human eye and the optical system of the instruments. It is for this reason that each user is encouraged to develop his own standards for performance. The stability test has been developed by statistical procedure for various environmental conditions.

Blood: This test is slightly more sensitive to free hemoglobin and myoglobin than to intact erythrocytes. The test is generally capable of detecting 0.015mg/dl free hemoglobin or 5 to 10 intact red blood cells per microliter urine. The sensitivity may be reduced in urines with high specific gravity and ascorbic acid content. The appearance of Green spots on the reagent test area indicates the presence of intact erythrocytes in the urine.

Bilirubin: The test has a sensitivity of 0.5mg/dl bilirubin. Bilirubin in urine indicates liver disease before any clinical signs are usually evident.

Urobilinogen: This test can detect urobilinogen in concentrations as low as 0.1 mg/dl (approximately 0.1EU/dl); therefore, most normal urines may give a slight pink reaction.

Ketones: The reaction of this reagent pad is caused by acetoacetic acid in urine, acetone or beta - hydroxybutyric acid makes no significant contribution to this test. Ordinarily, the reagent area detects 5.0mg of acetoacetic acid in 100ml urine. Some high specific gravity and low pH urines may give reactions up to and including trace level (5.0mg/dl).

Protein: The test is more sensitive to albumins than to gamma - globulins, Bence - Jones proteins, and mucoproteins; such proteins do not interfere with the reaction of albumin.

Nitrite: This test has a sensitivity of 0.05mg/dl nitrite ion or the amount of bacteria about 10⁵/dl in urine of normal specific gravity and moderate levels of ascorbic acid. The test is specific for nitrite and independent of urinary pH of any other substance normally excreted in urine. Comparison of the reacted area against a white background may aid in the detection of low levels on nitrite.

Glucose: The test has a sensitivity of 50-100mg glucose in 100ml urine, and is specific for glucose. No substance excreted in urine other than glucose is known to give a positive result. False negative results may be obtained with the presence of levodopa, ascorbic acid, glutathione, and dipyrone. If the test color appears somewhat mottled at the higher glucose concentrations, match the darkest color to the color blocks.

pH: This test produces distinct color changes from orange to blue over the pH value 5 - 9. Values will be read to within 1 unit; however, an accurate reading may be confused because of slight variations caused by the pigments in the urine.

Specific Gravity: This test permits determination of urine specific gravity of 1.000, 1.005, 1.010, 1.015, 1.020, 1.025 and 1.030. Highly buffered alkaline urines may cause low reading of result.

Leukocytes: The test is generally capable of detecting 20 - 25WBC/ μ l as a trace.

BIBLIOGRAPHY:

1. NCCLS. Protection of Laboratory Workers from infectious Disease Transmitted by Blood and Tissue, NCCLS Doc. M29-P, 7.9 May:342-347 1985.
2. Kaplan L.A. and Pesce A.J.; Clinical Chemistry Theory, Analysis and Correlation; C.V.Mosby; pp 1004-1007;1984
3. Henry, J.B. et.al: Clinical diagnosis and Management by Laboratory methods, 16th ed, Philadelphia: Saunders; 1979; pp.579-608.
4. Paterson,P.et.al: Maternal and Fetal Ketone concentrations in Plasma and Urine, Lancet: 862-865.; April 22, 1967.

GENERAL REFERENCES:

1. Free,A.H. and H.M.Free; Urinalysis, Clinical Discipline of Clinical Science, CRC Crit. Rev.Clin.Lab.Sci, 3(4); 481 - 531; 1972
2. G(KERN=65532)raff,L.;A Handbook of Routine Urinalysis, Philadelphia,J.B.Lippincott Co.,(1/3)1983
3. Jungreis,E:Spot Test Analysis,N.Y.; John Wiley & Sons; 1985
4. Kark, R.M.et.al; A Primer of Urinalysis, 2nd ed, N.Y.; Harper and Row; 1963
5. Scheer, W.D., Am. J. Clin. Pathol., 87, 86 - 93(1987)



Imported by
Clonal Technologies, Australia
1300 795 335
www.clonaltech.com.au



Manufactured by
ChungDo Pharm.Co.,Ltd
Seoul, Korea.



Obelis SA
Av. de Tervueren
BTE 44, B-1040
Brussels, Belgium